




# AMX Medical Systems


An ISO 9001-2008 Certified Company

OPEX - 1

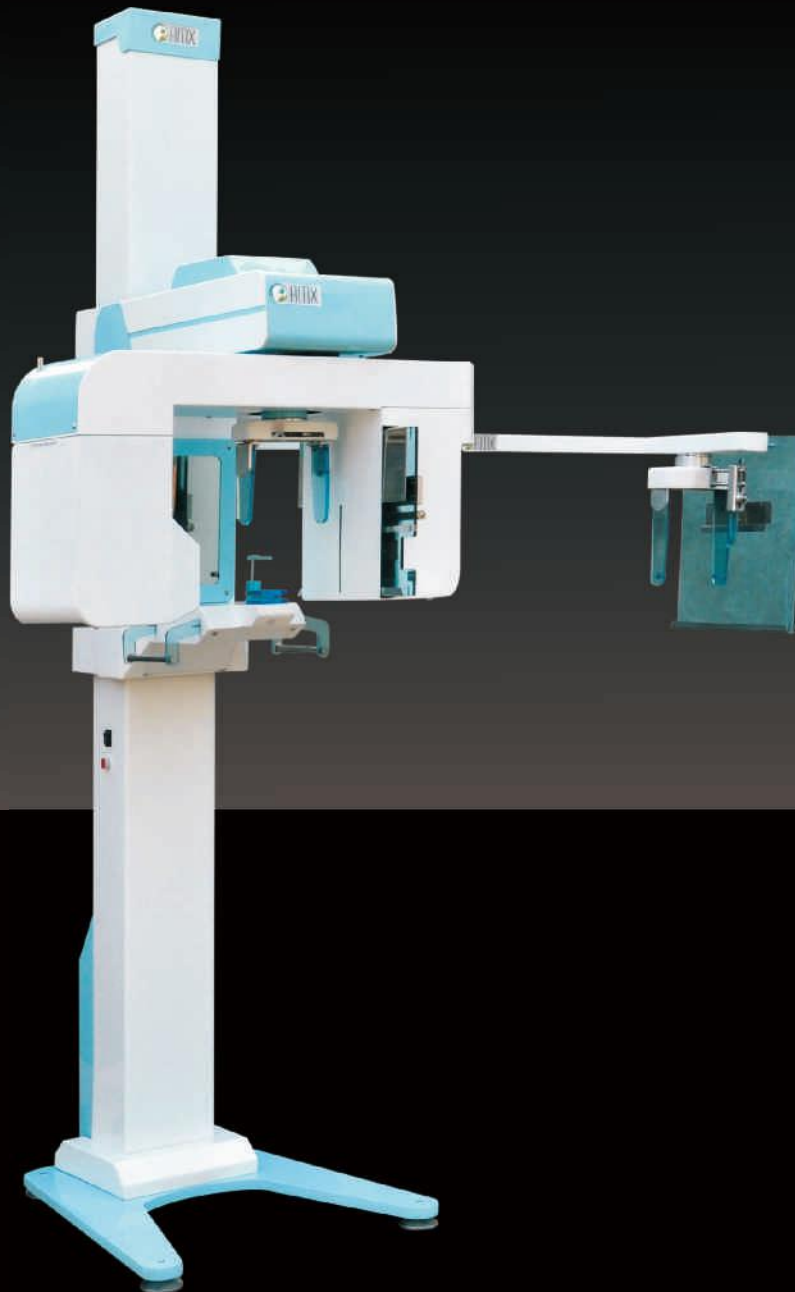

Changing The world  
for a **Better**

**Life**

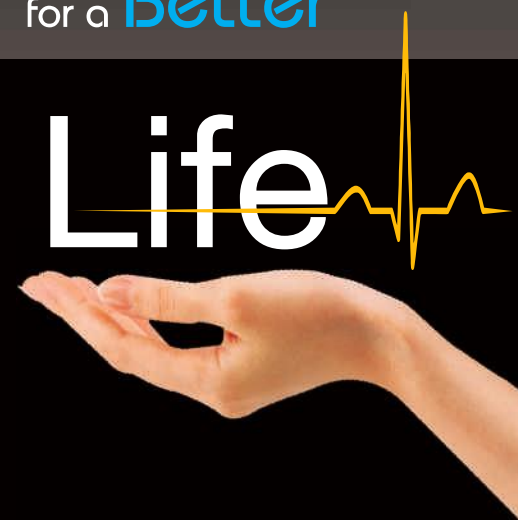

[www.amxmedicalsyste.ms.in](http://www.amxmedicalsyste.ms.in)



## TECHNICAL SPECIFICATION

Power Supply	230+10%, 10 AMP
Column Height	230 cm
Anode Voltage	52 KVP to 85 KVP in step of 2 KVP
Vertical Movement	Actuator Driven
Tube Current	8,9 and 10mA Stations
X-ray Tube	0.5 mm sq. Fine focus
Exposure Time	OPG-17 Sec. For Adult-14 sec. Child CEPH - 0.2 sec to 3 sec. TMJ - 4x4 sec.
Film Size	OPG & TMJ - 6"x12" & 10"x12" CEPH - 8"x10"
Cassette Size	OPG & TMJ - Flat 6"x12" & 10"x12" CEPH - Flat 8"x10"
Safety Features	Provision for Earth Fault, KV Error, Filament Error & Thermal Protection



## AMX Medical Systems

An ISO 9001-2008 Certified Company

### Corporate Office :

441, Pocket GH - 5 & 7, Paschim Vihar,  
New Delhi - 110087 (INDIA)  
Mobile : +91-9718265567

### works :

74, Mainapur Industrial Area, Meerut Road,  
Ghaziabad 201001, UP (India)  
Mobile : +91-9313299920

Email : [amxmedicalsistemas@gmail.com](mailto:amxmedicalsistemas@gmail.com) Website : [www.amxmedicalsistemas.in](http://www.amxmedicalsistemas.in)